

FIG. 2A

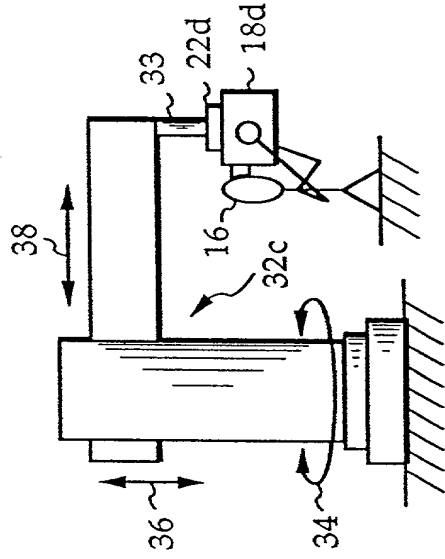


FIG. 4

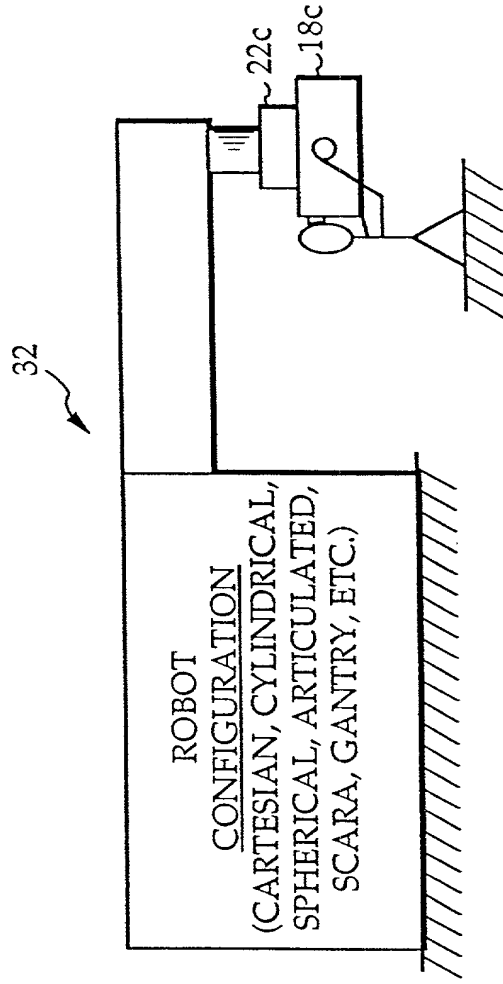


FIG. 3

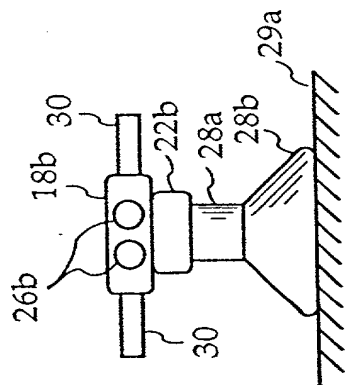


FIG. 20

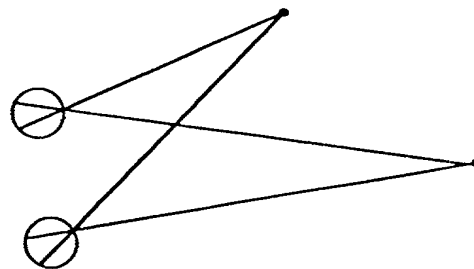


FIG. 20

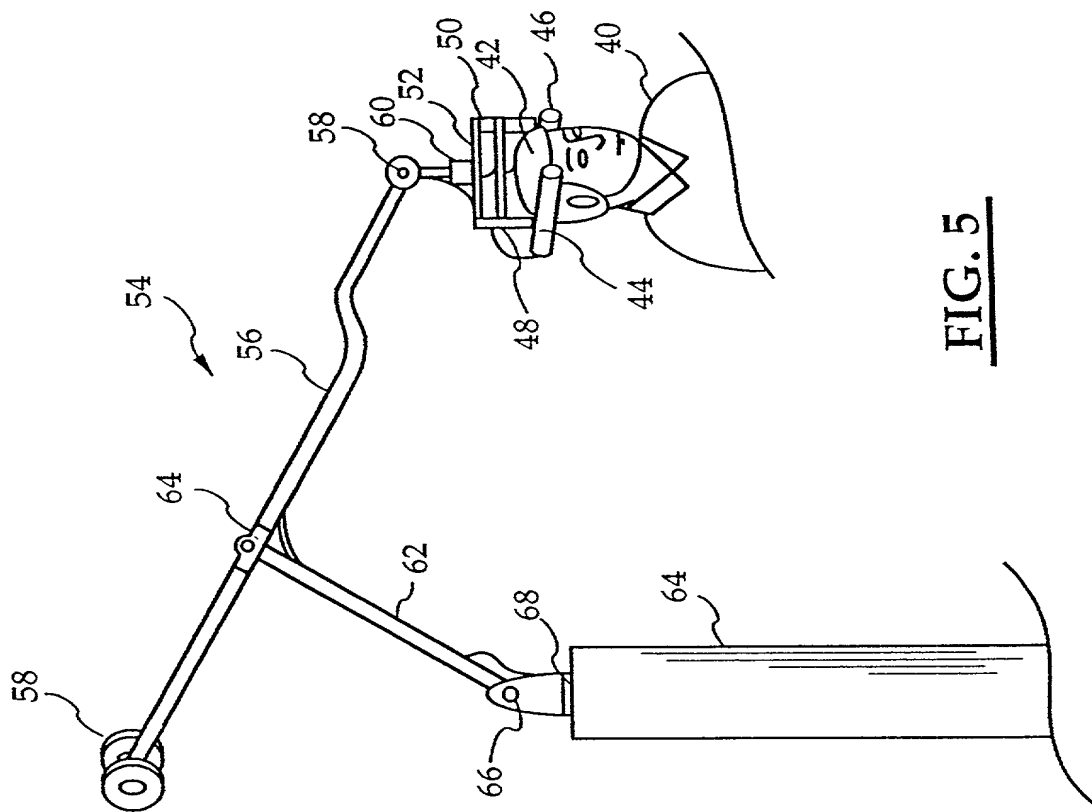


FIG. 5

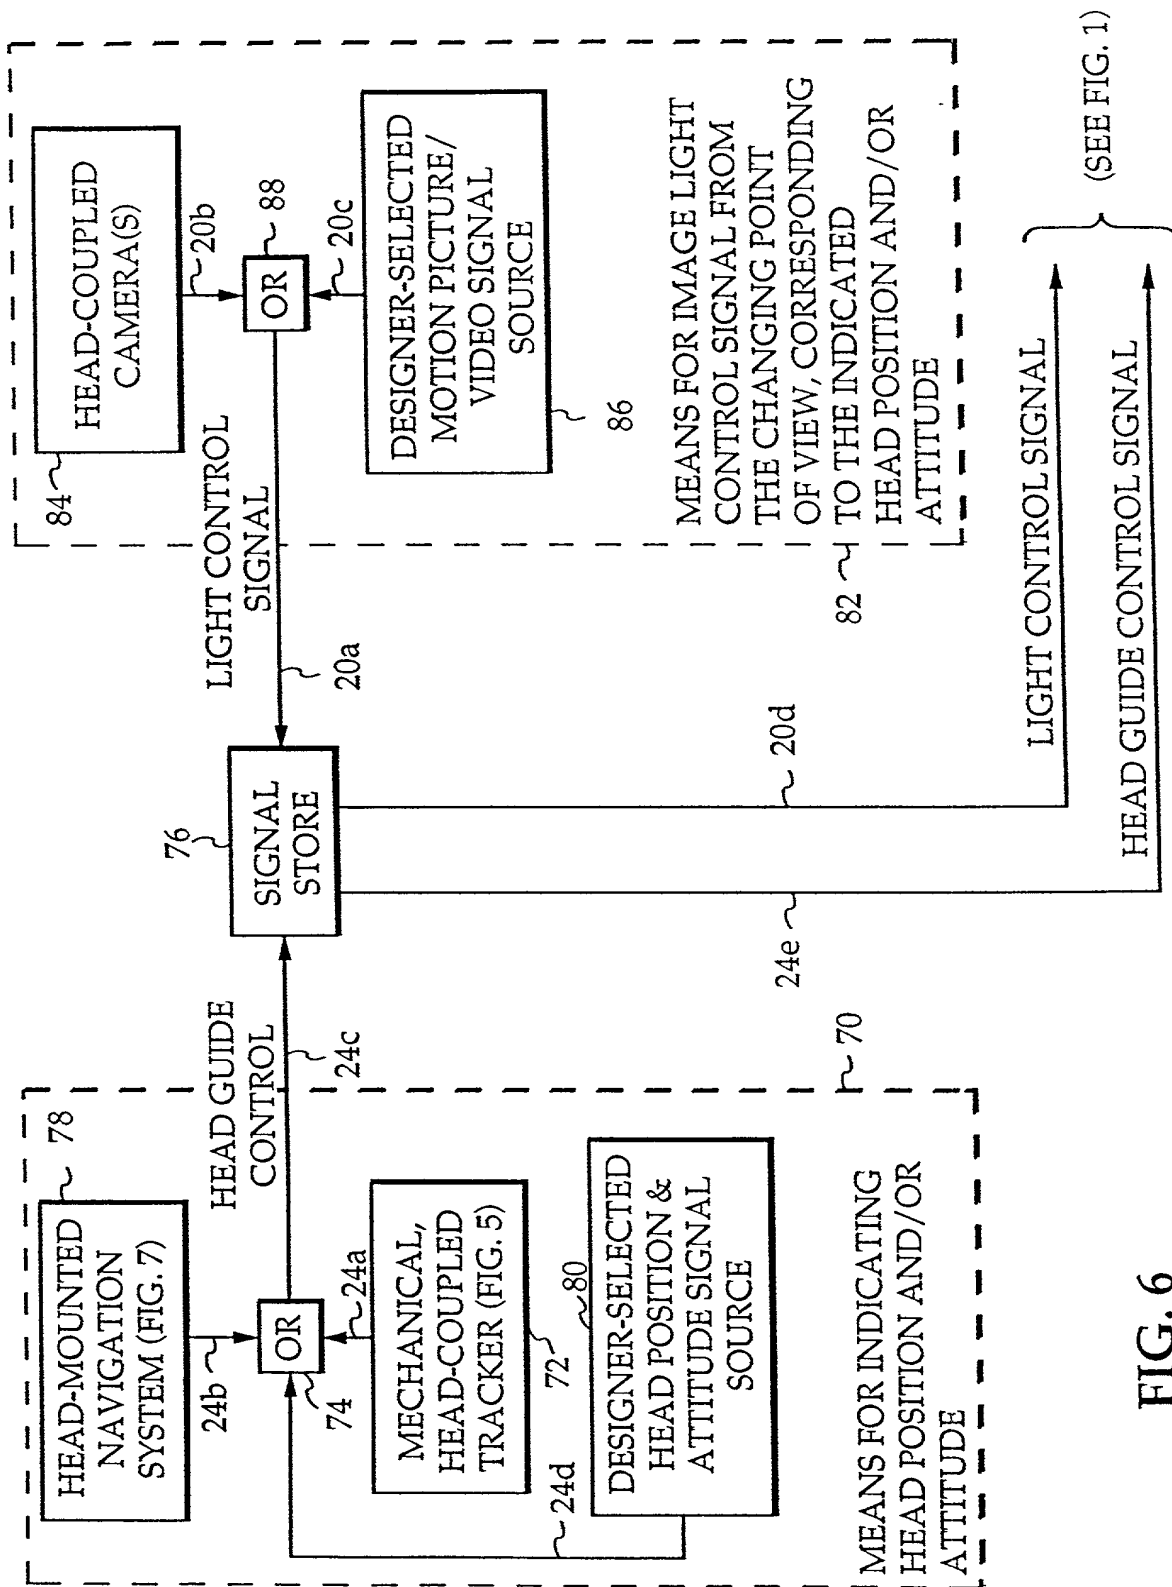


FIG. 6

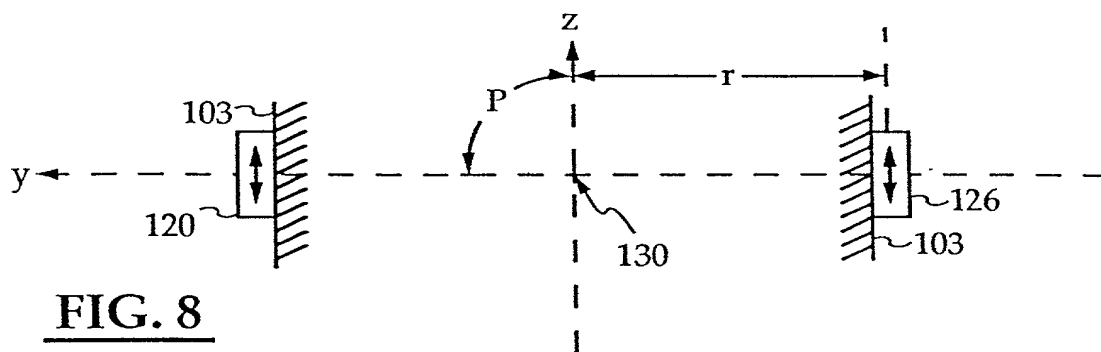
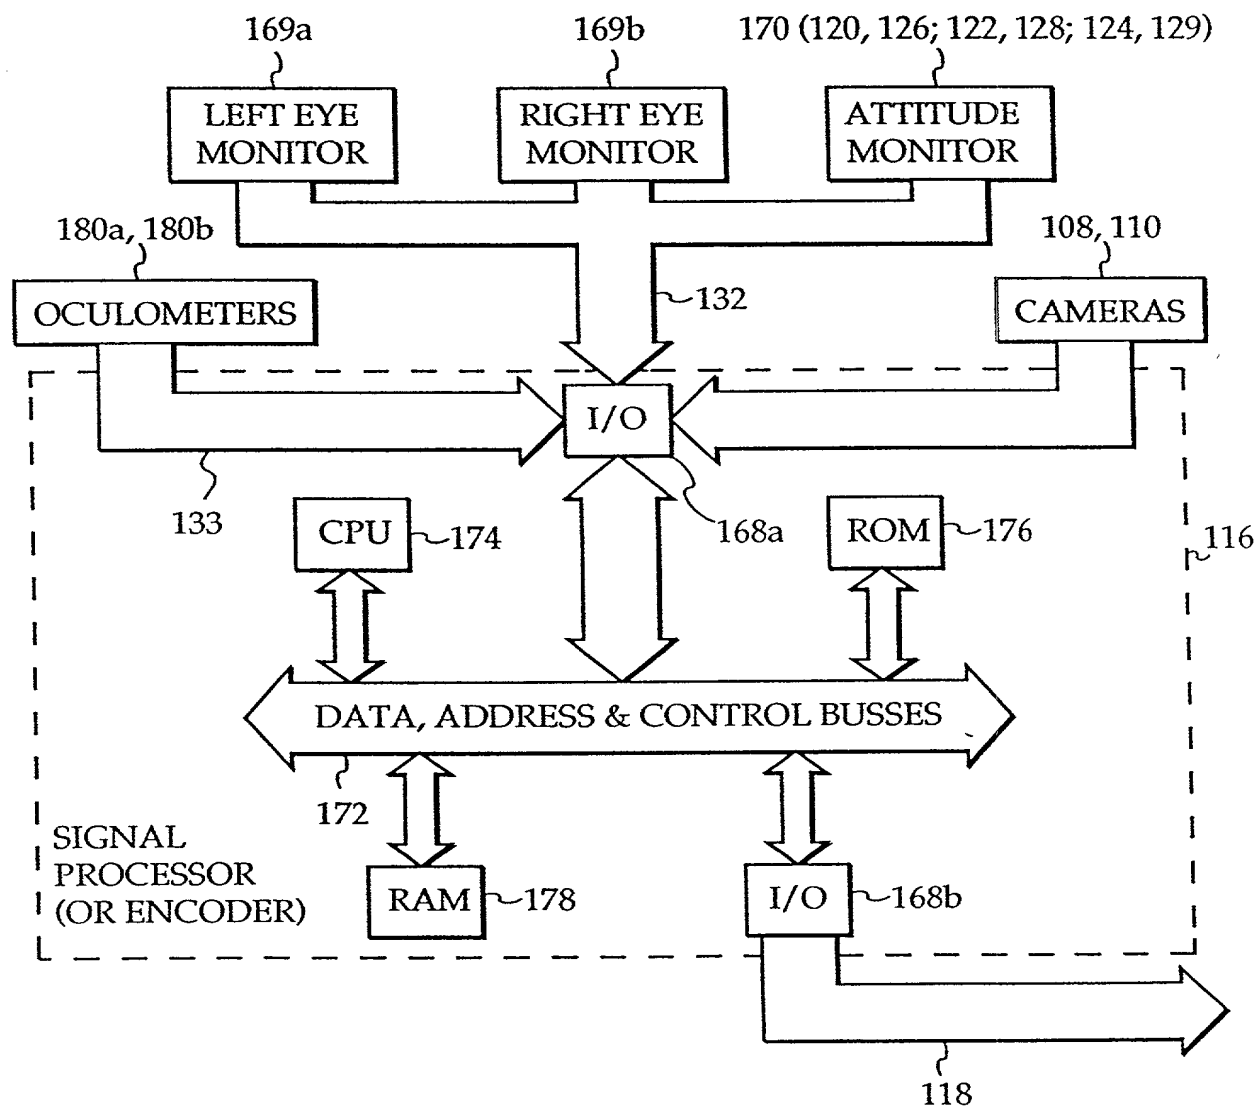


FIG. 12



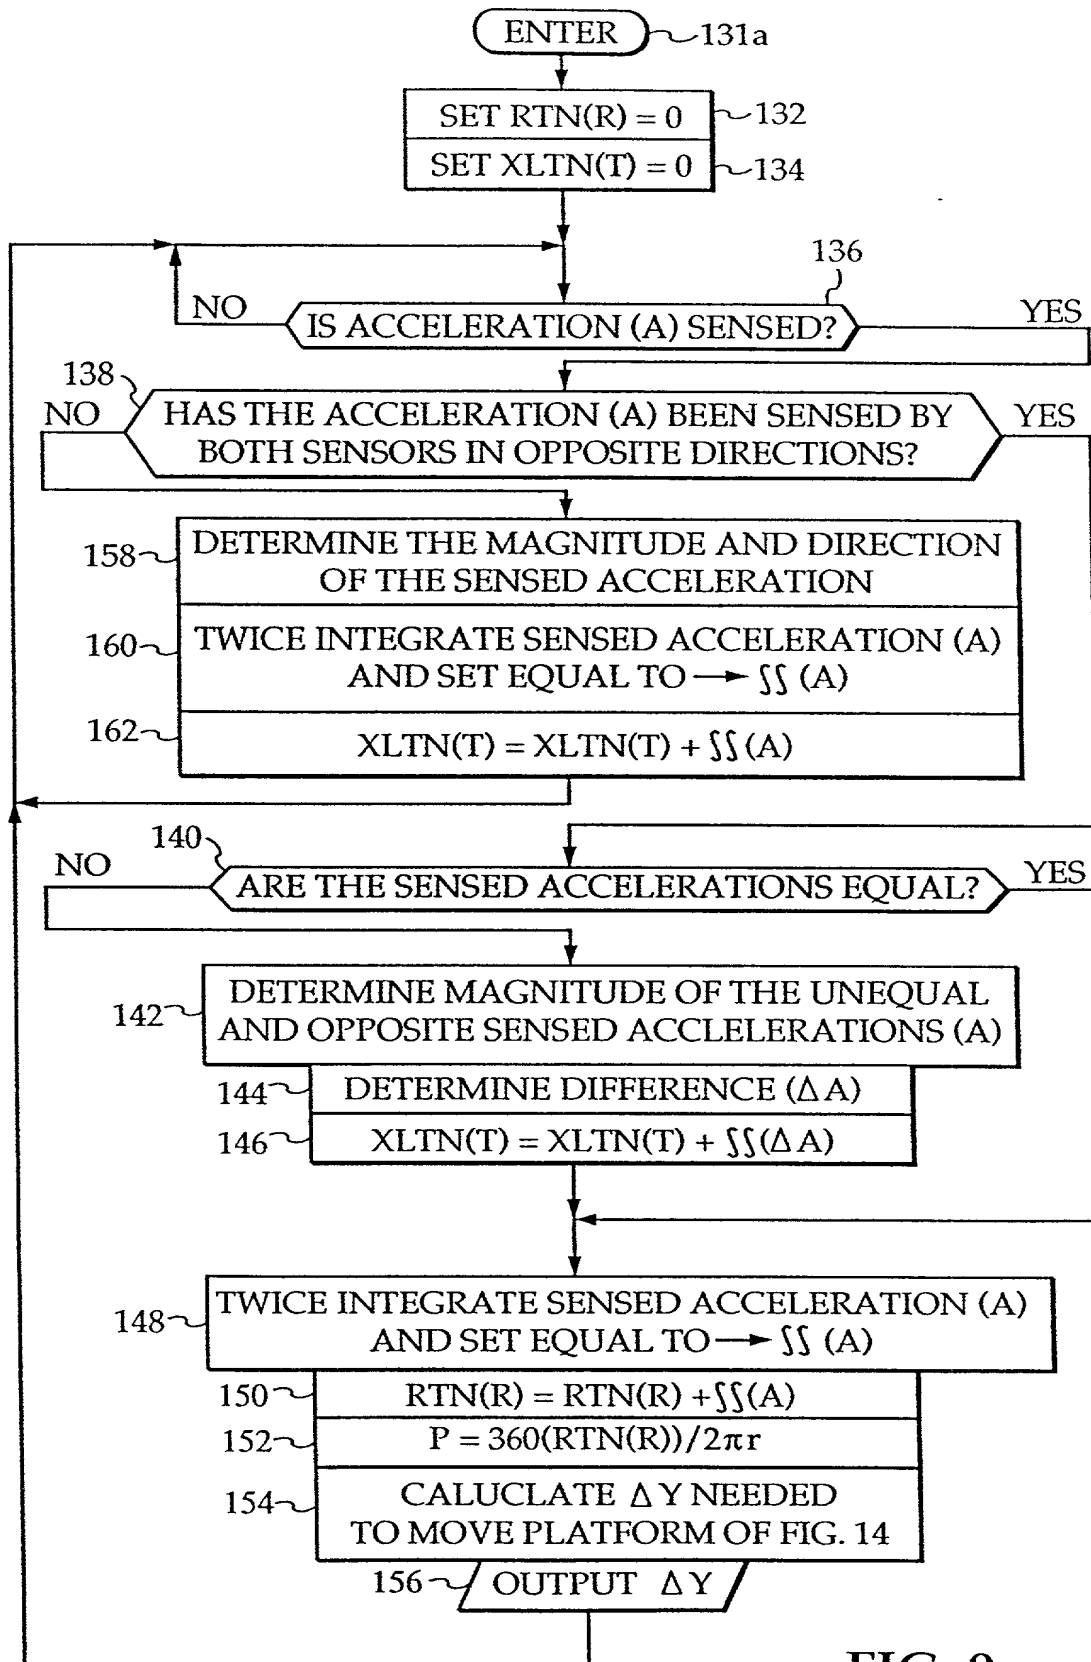


FIG. 9

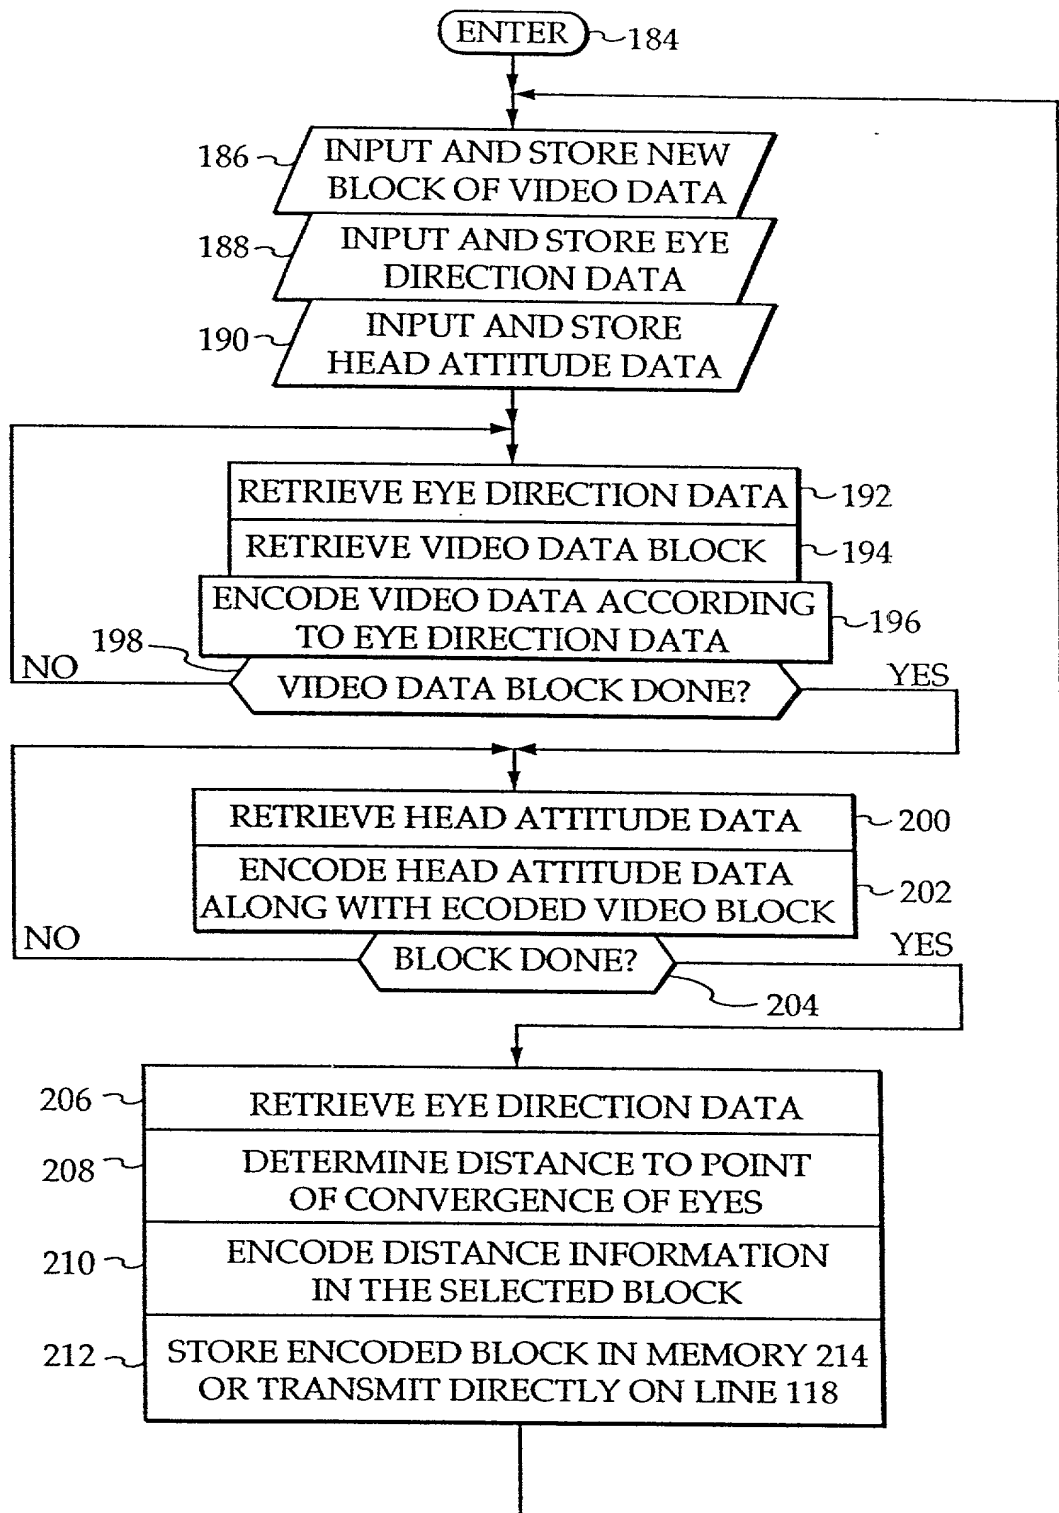


FIG. 10

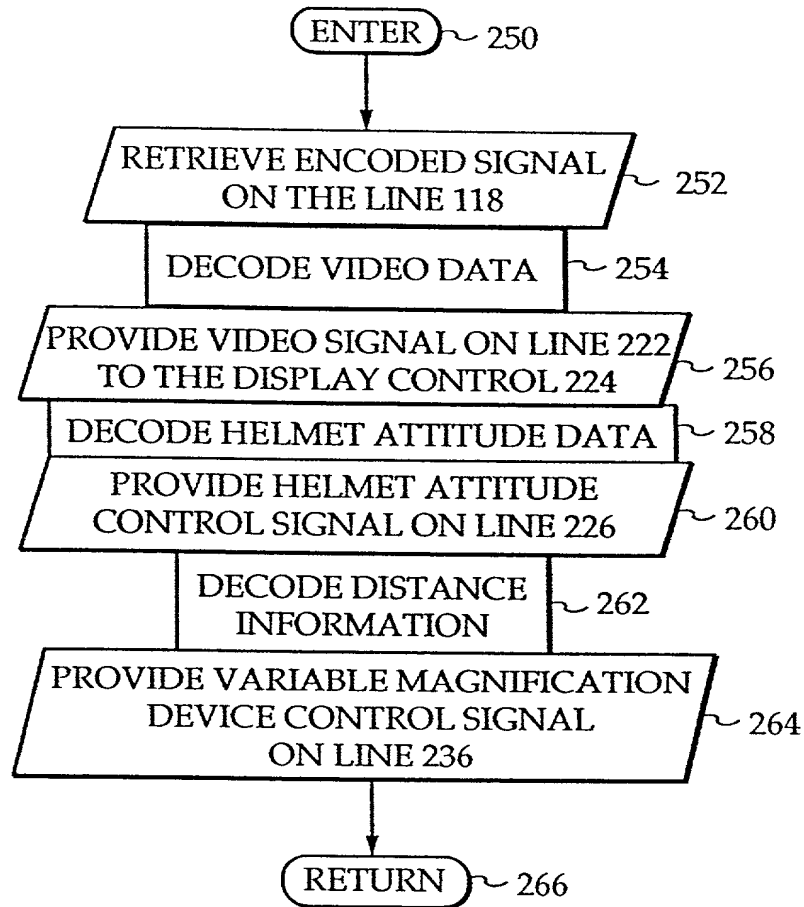


FIG. 11

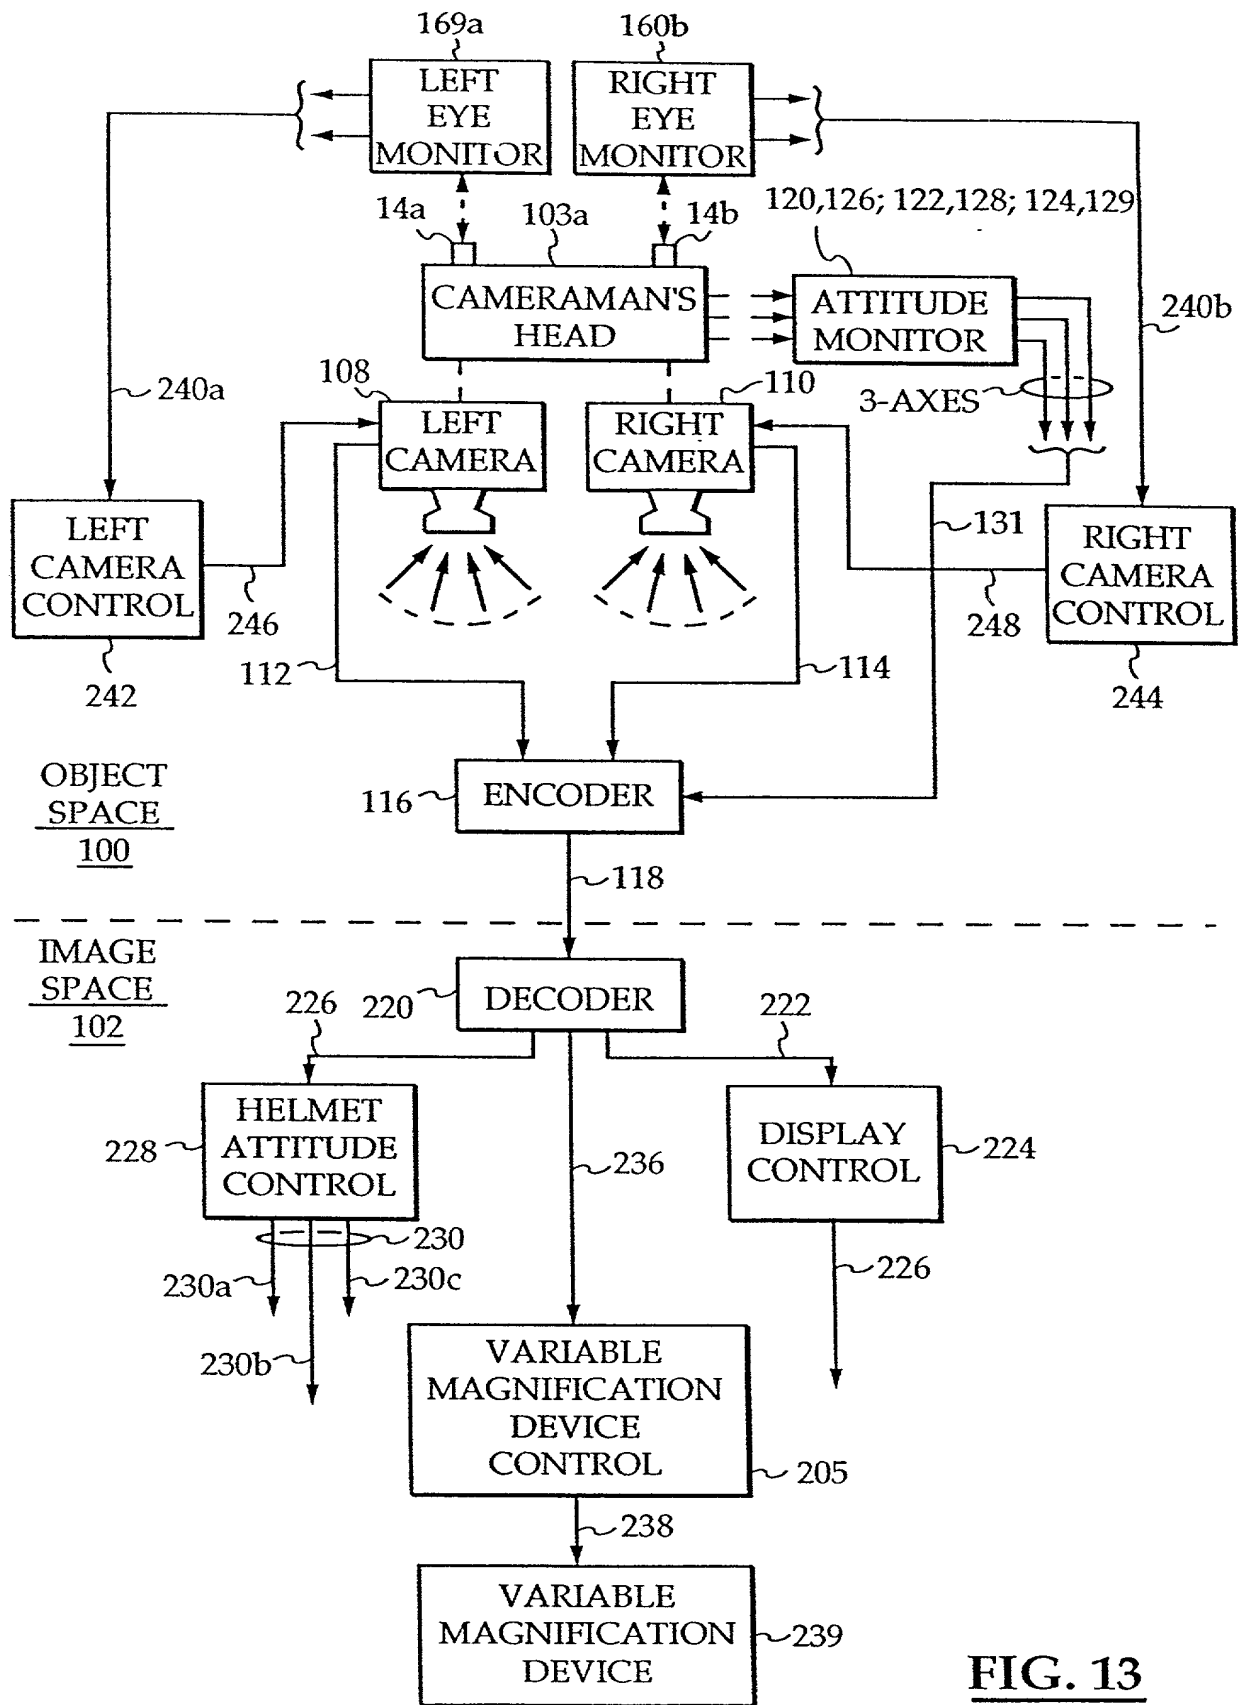


FIG. 13

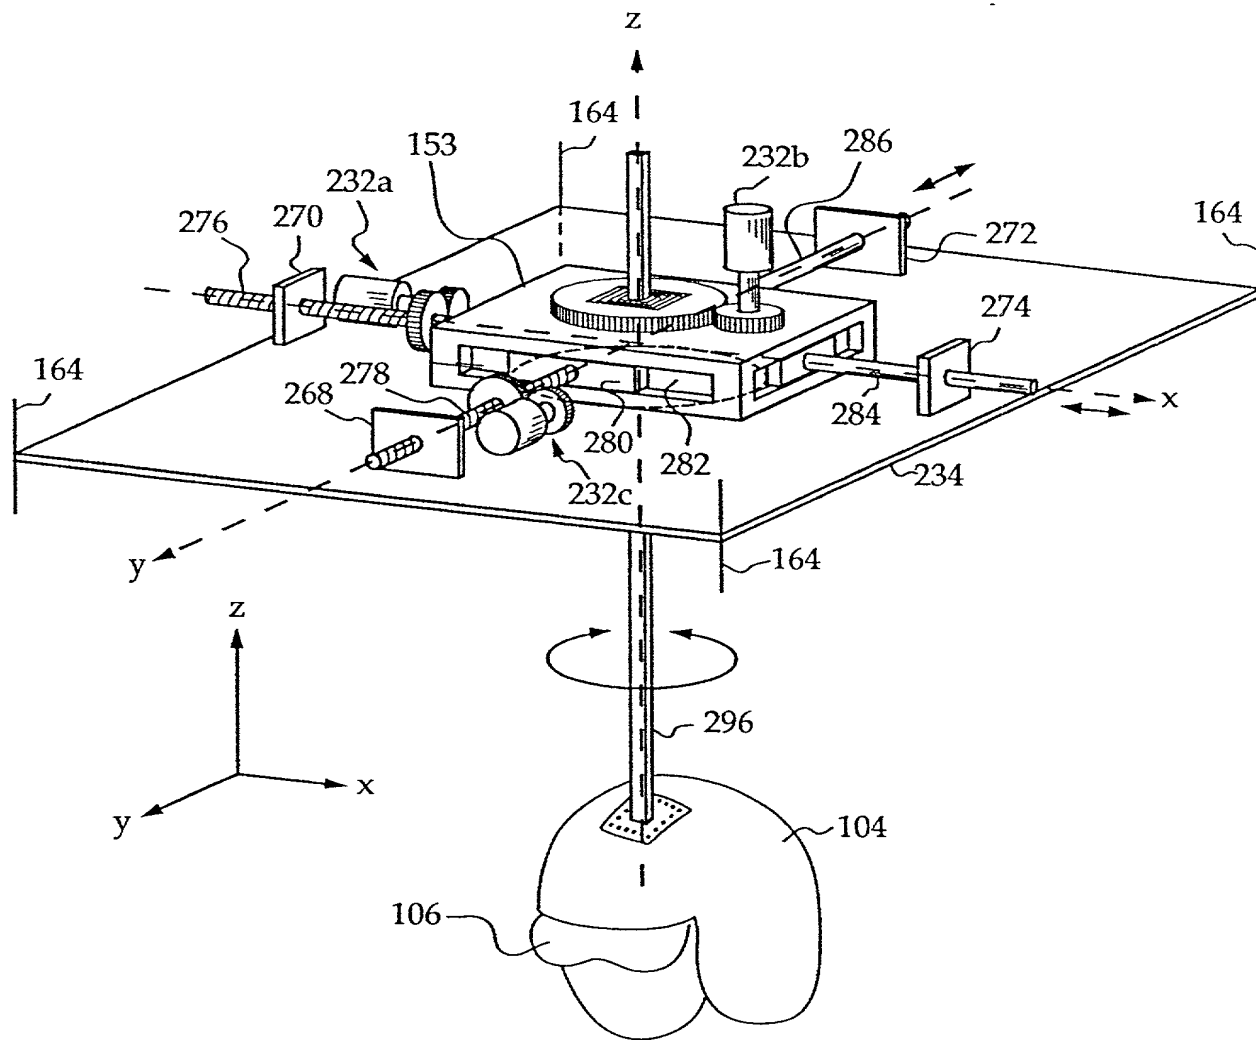


FIG. 14

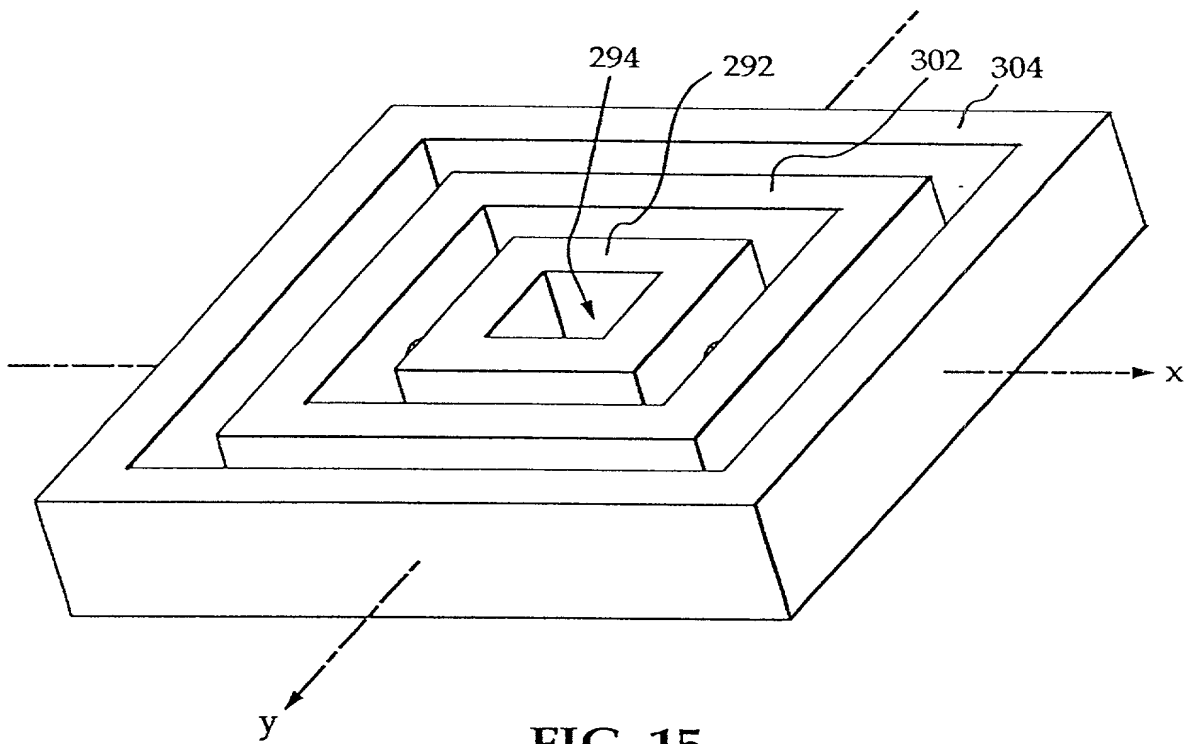


FIG. 15

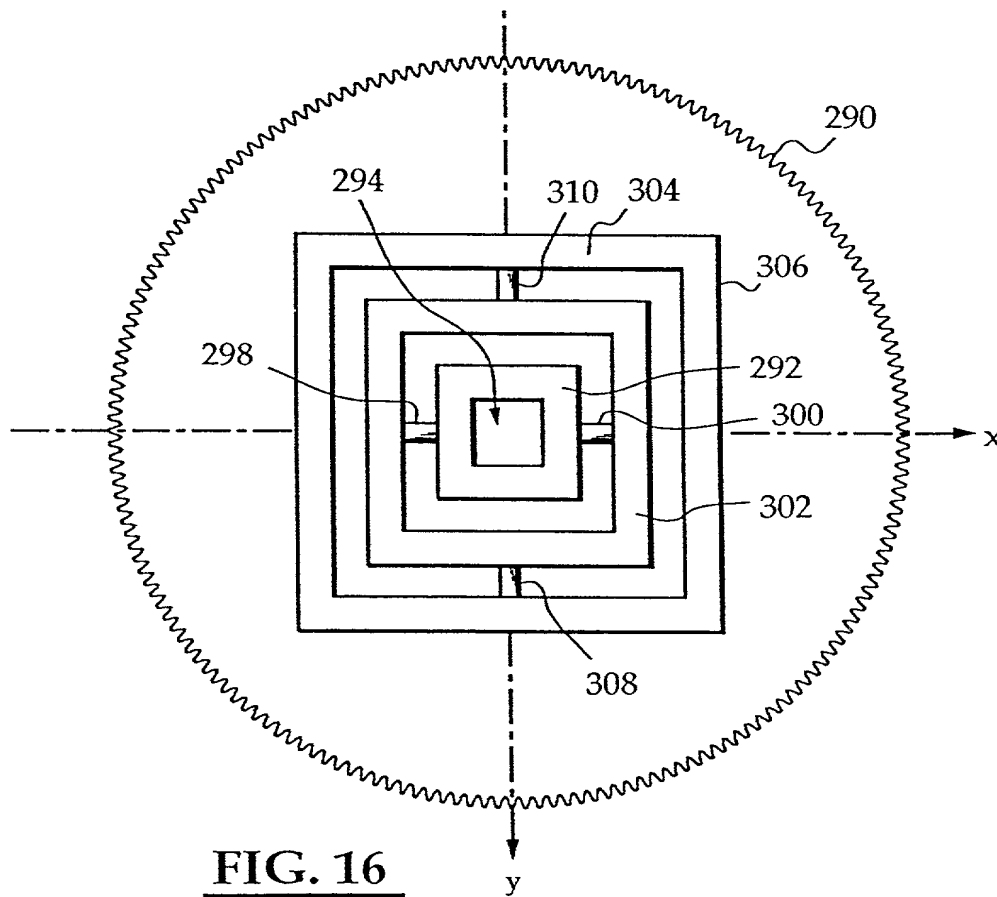
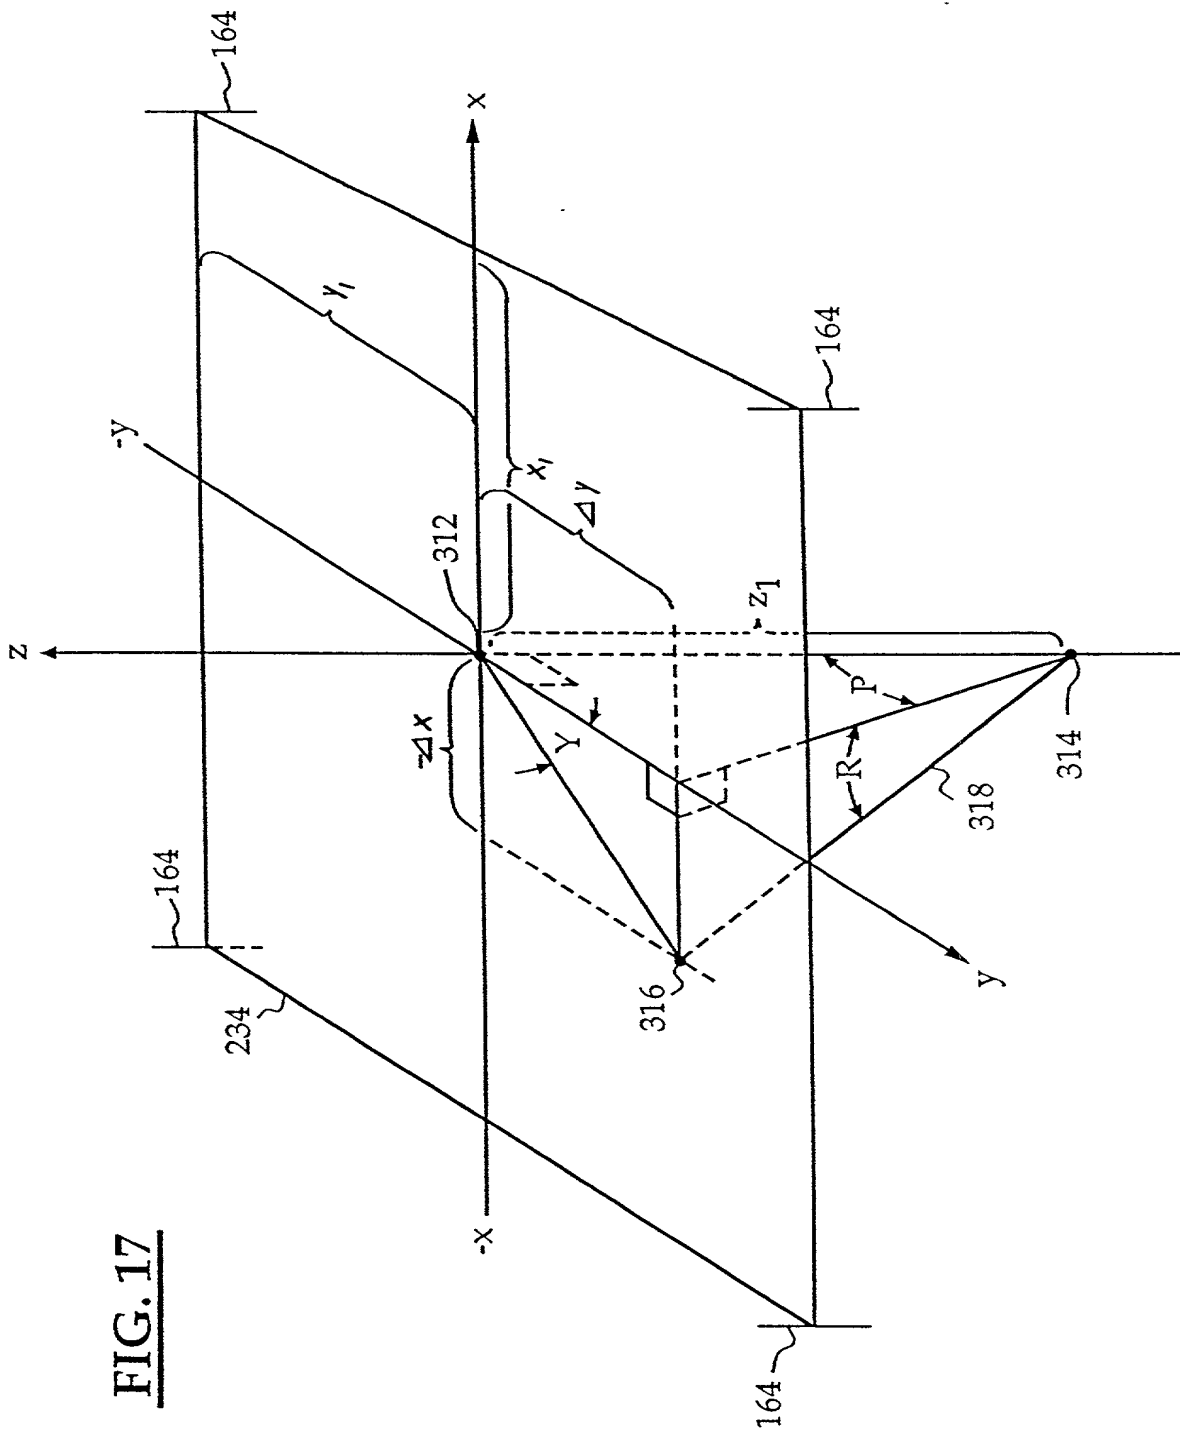


FIG. 16



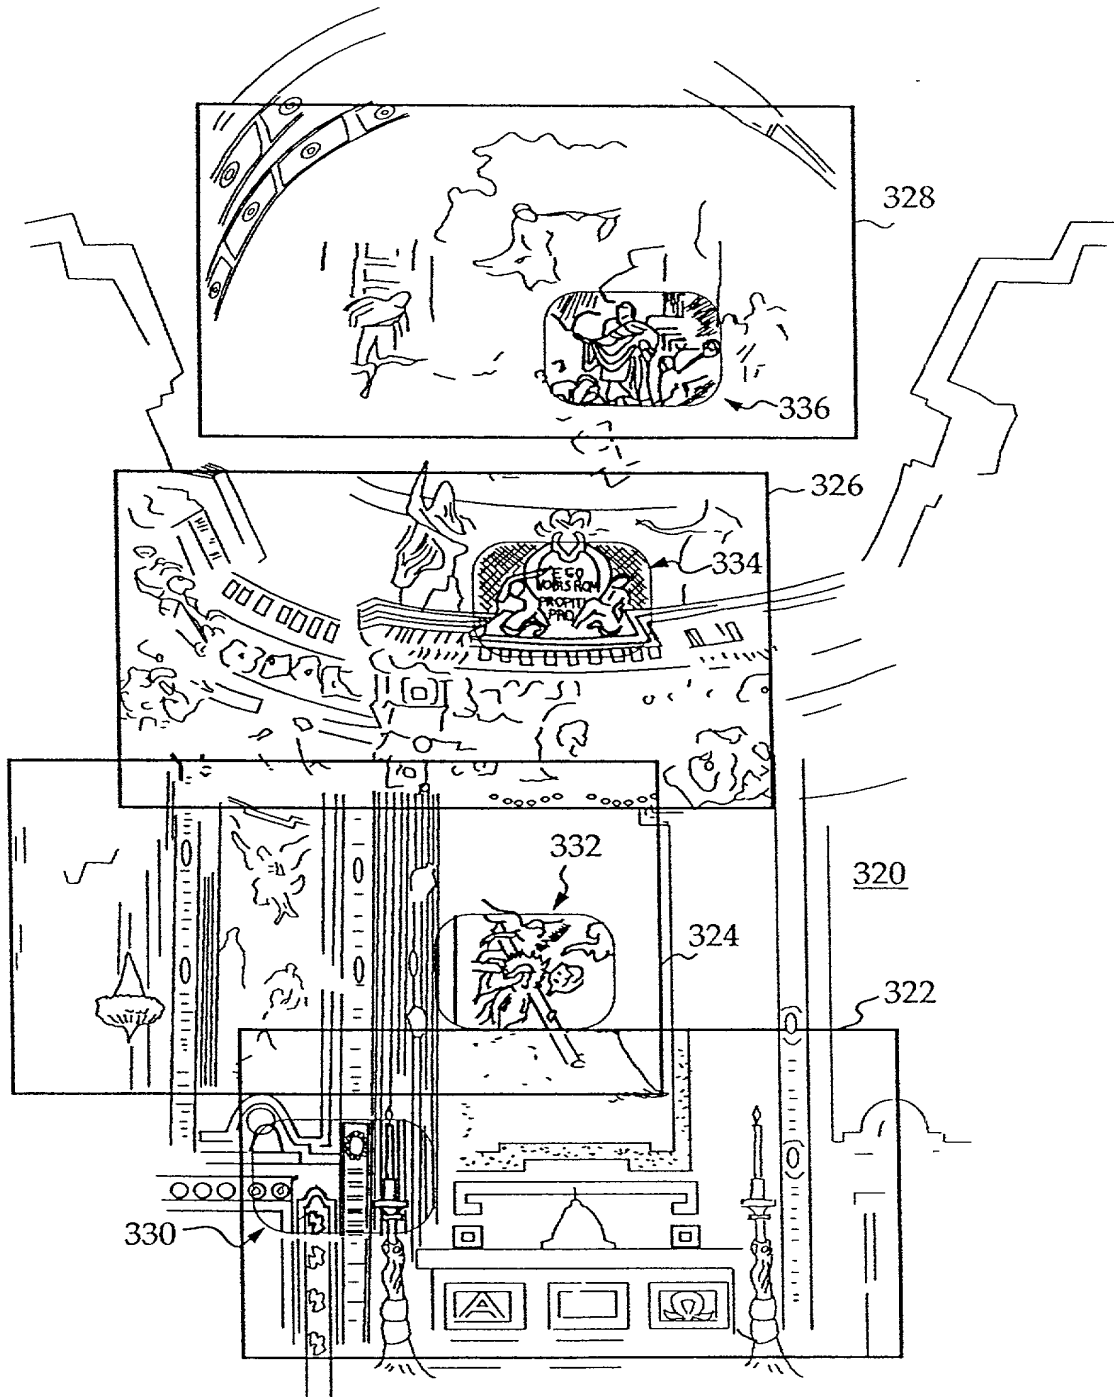


FIG. 18

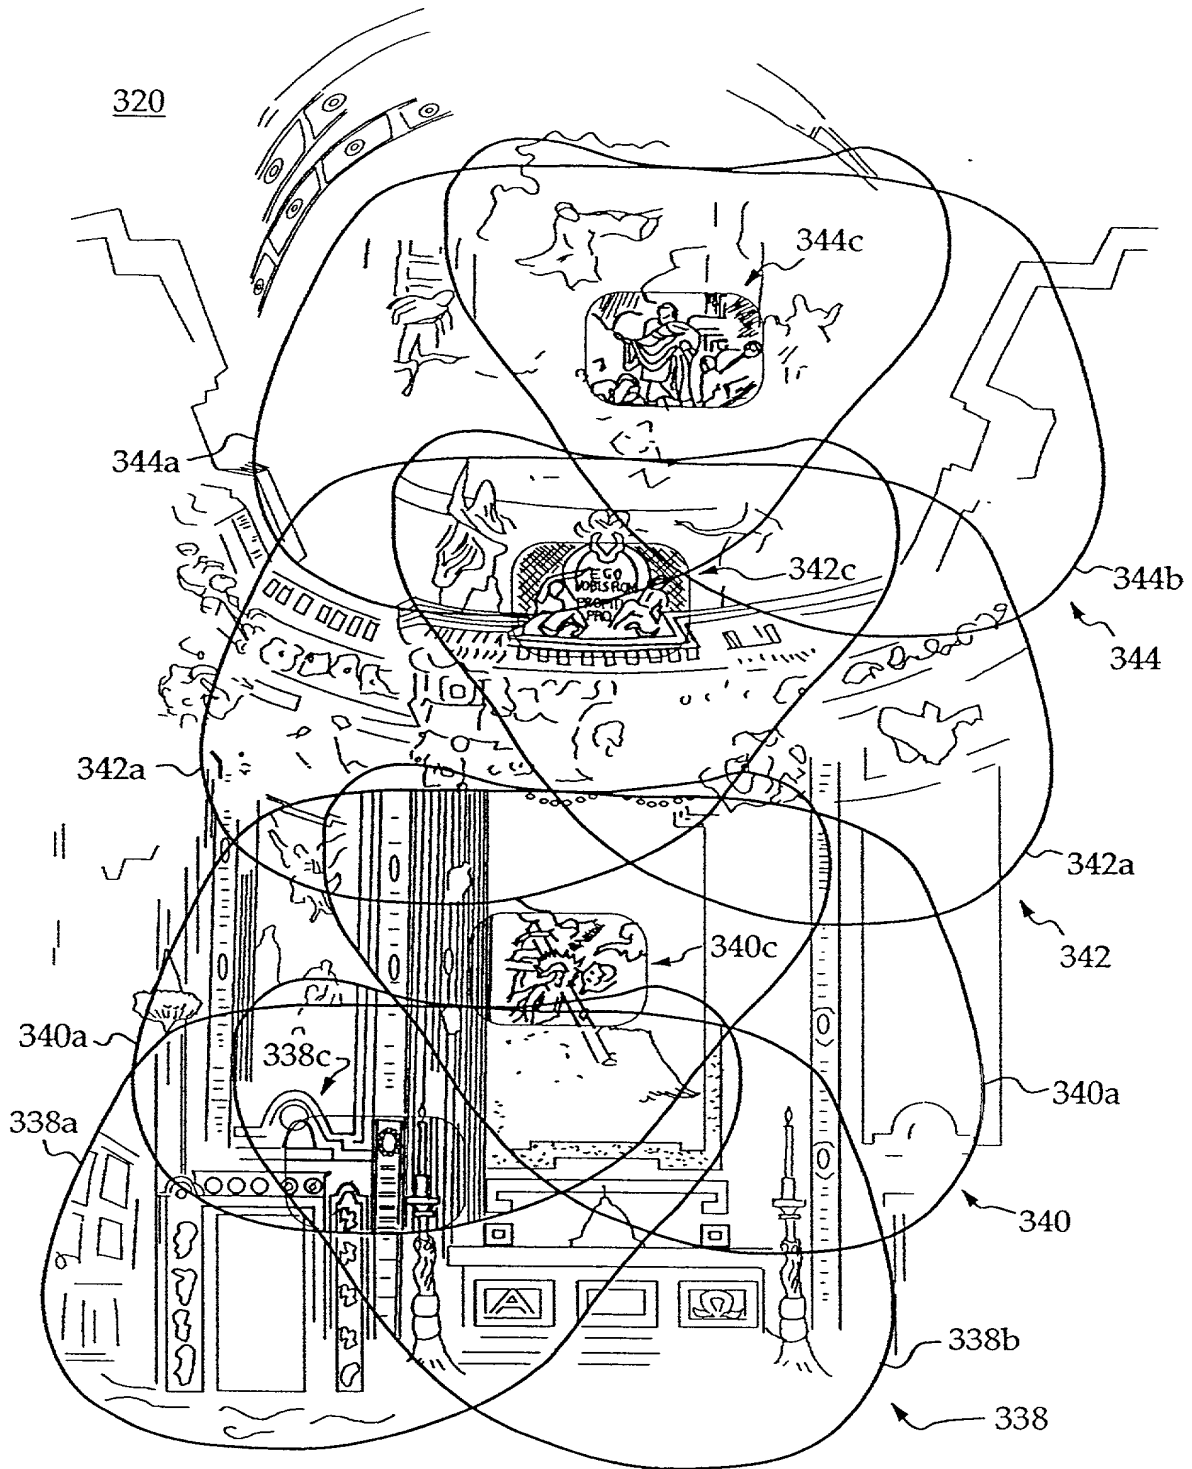


FIG. 19

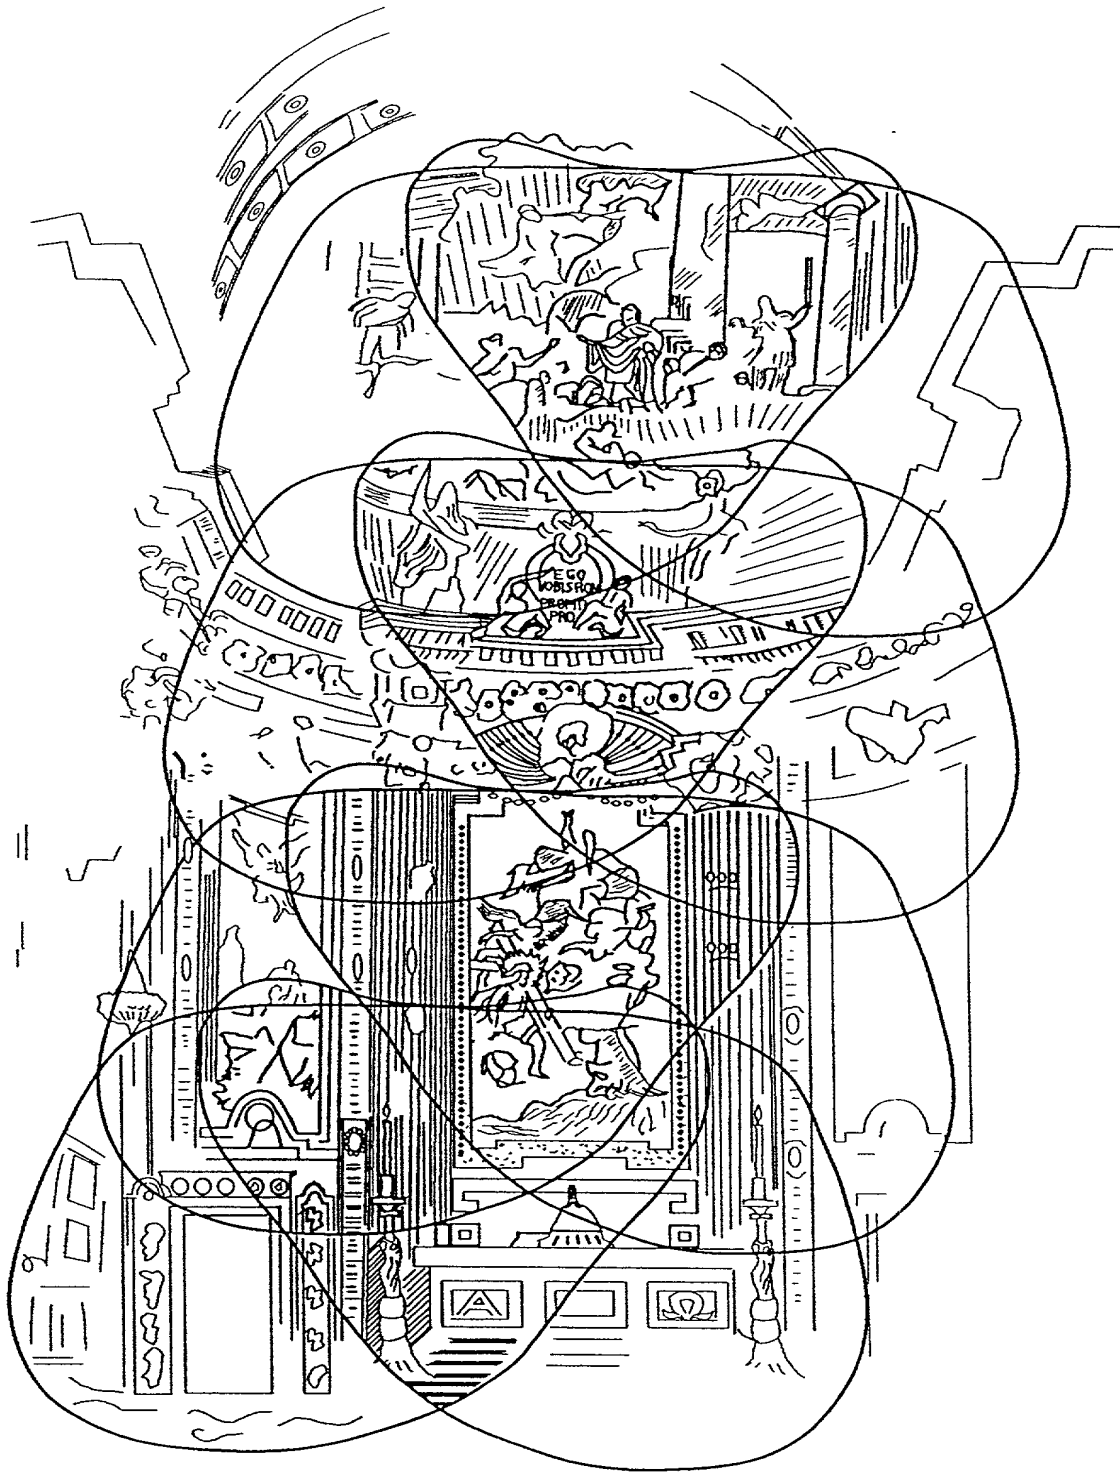


FIG. 21

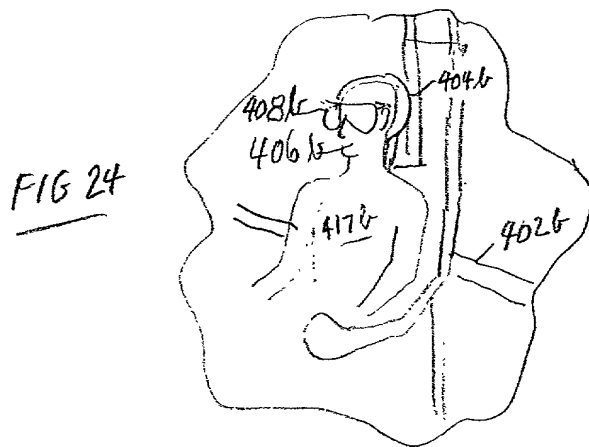
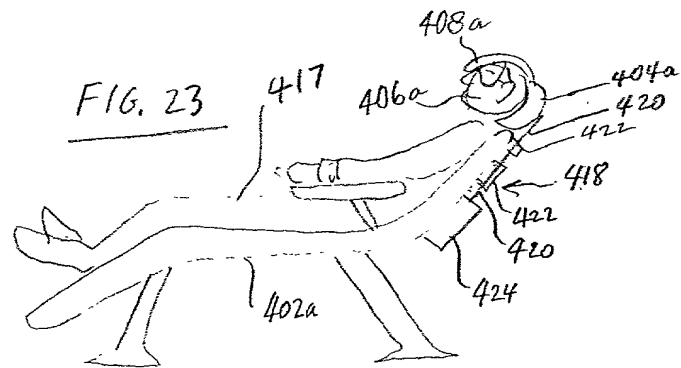
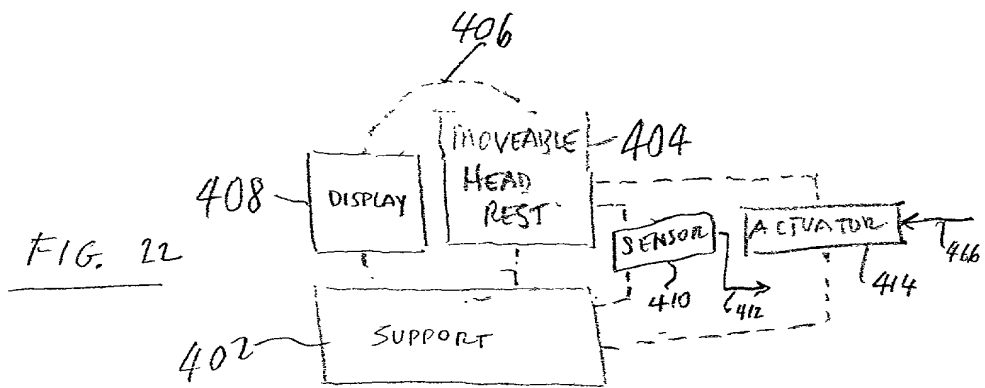


FIG 25

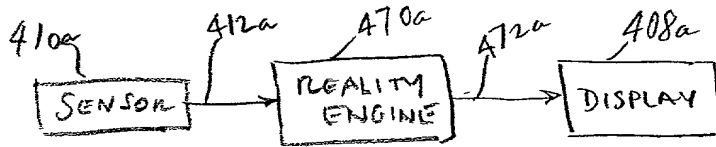
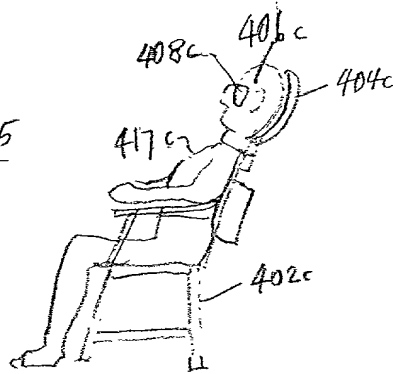


FIG 32

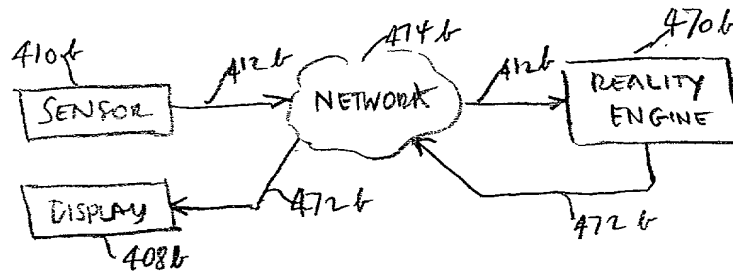


FIG 33

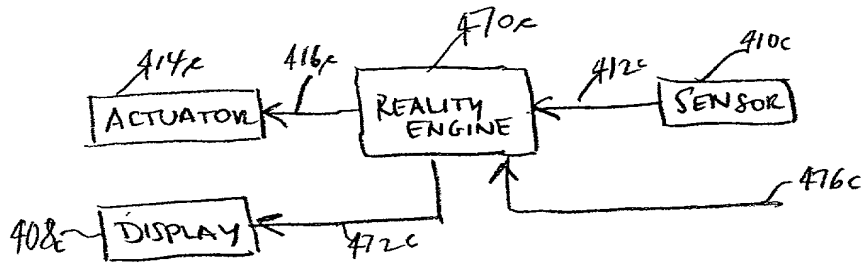


FIG 34

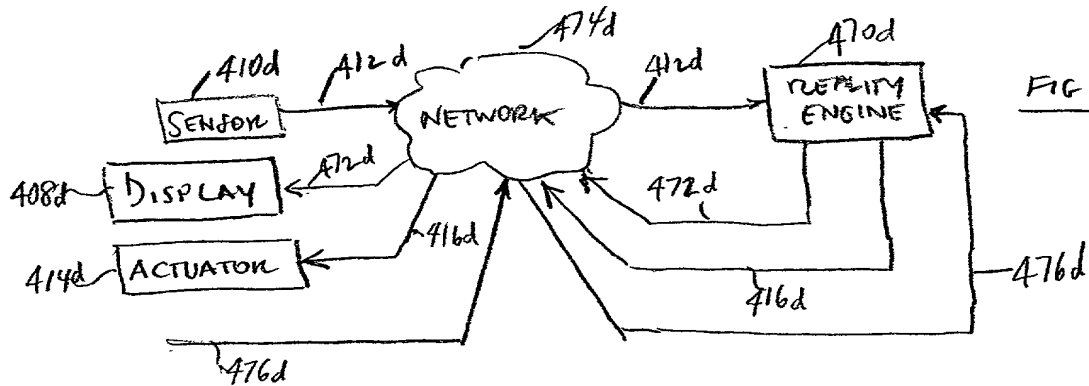


FIG 35

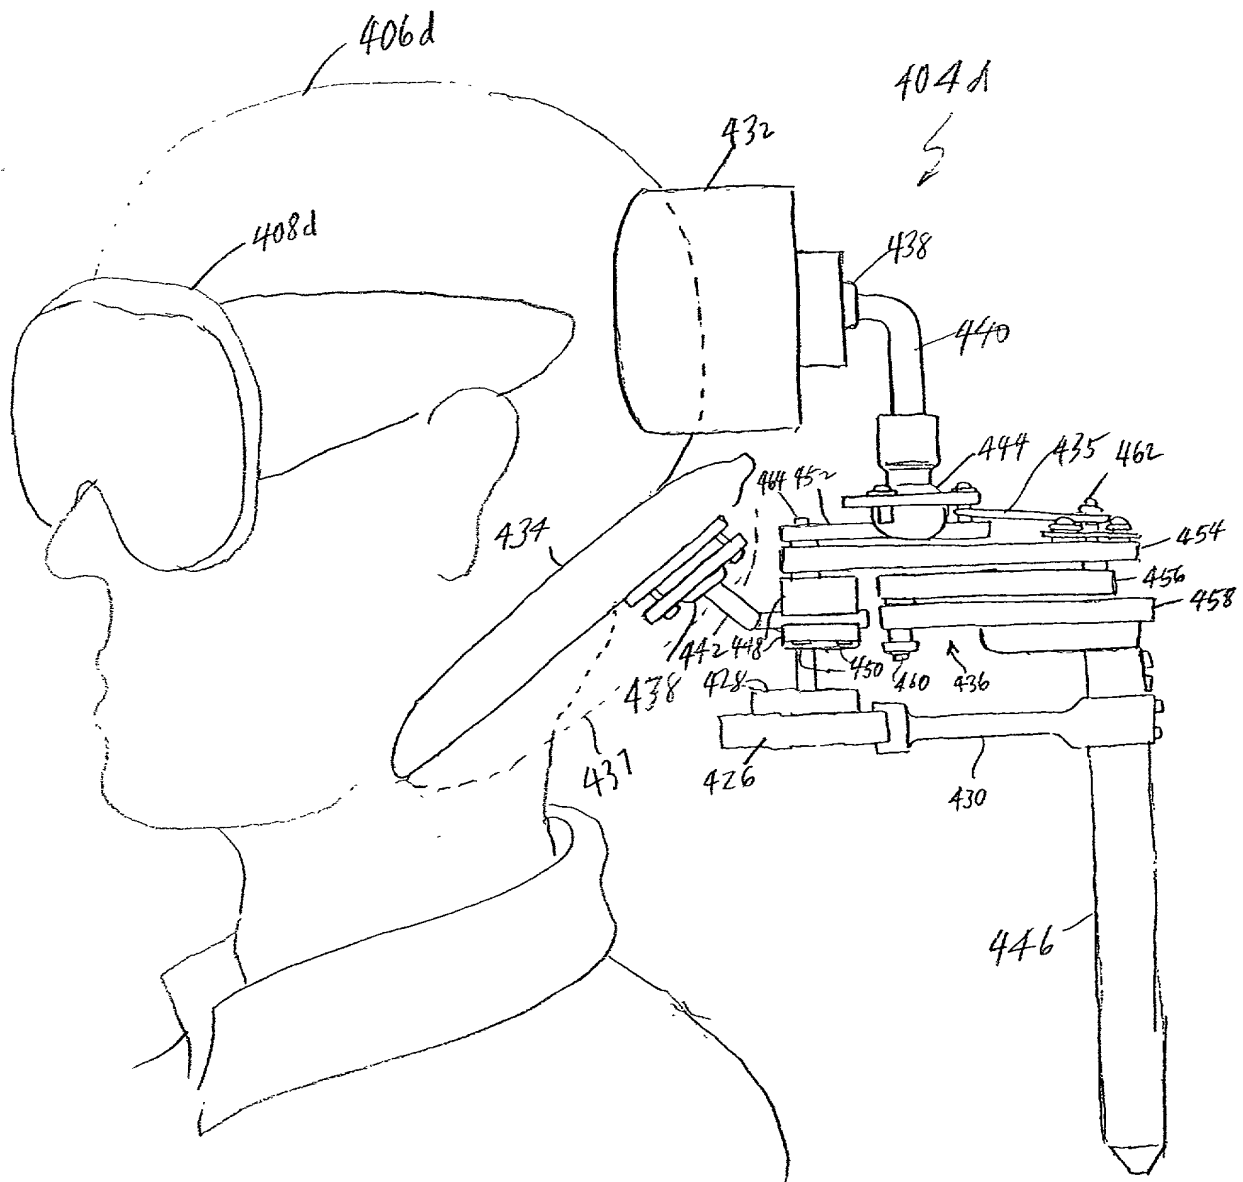


FIG 26

FIG. 27 is a cross-sectional view of the device of FIG. 26, taken along line 27-27 of FIG. 26.

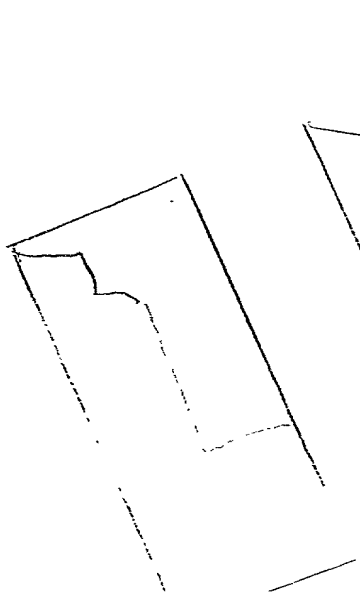


FIG 27

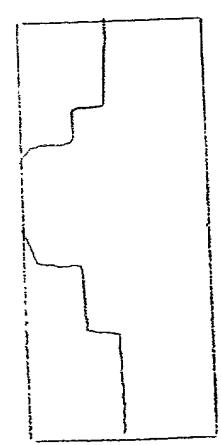


FIG 28




FIG 29

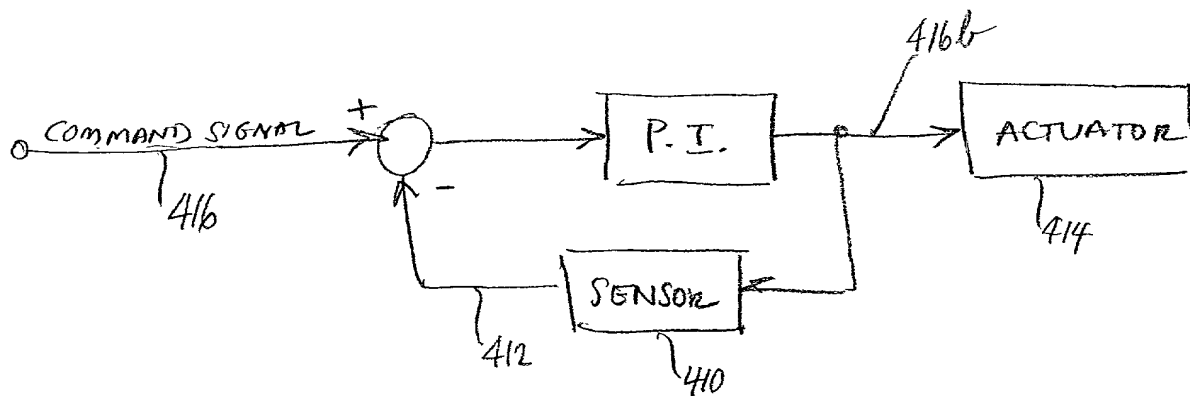


FIG. 31

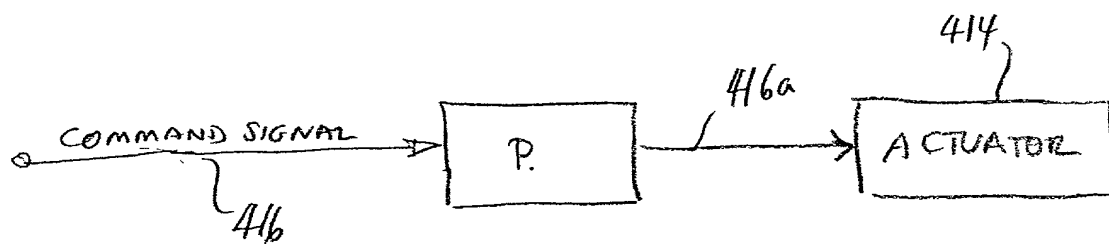


FIG. 30

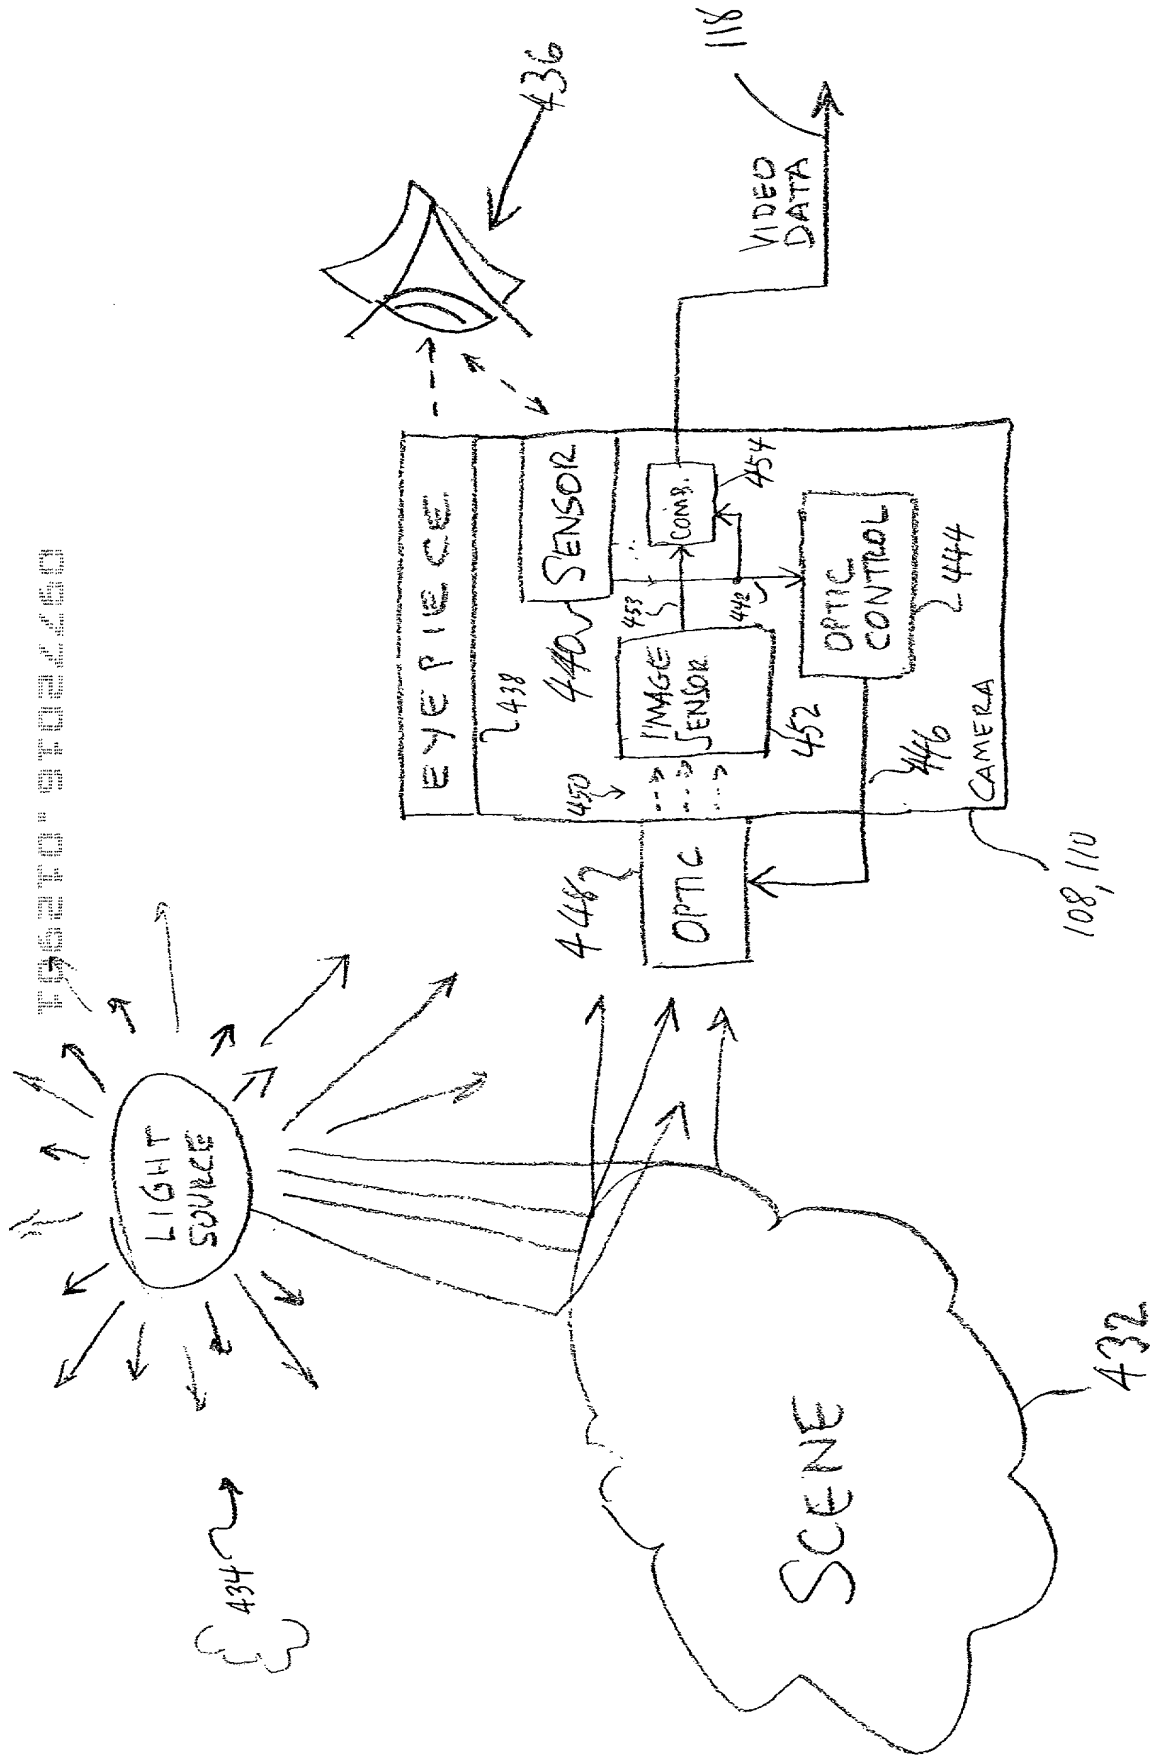


FIG 36

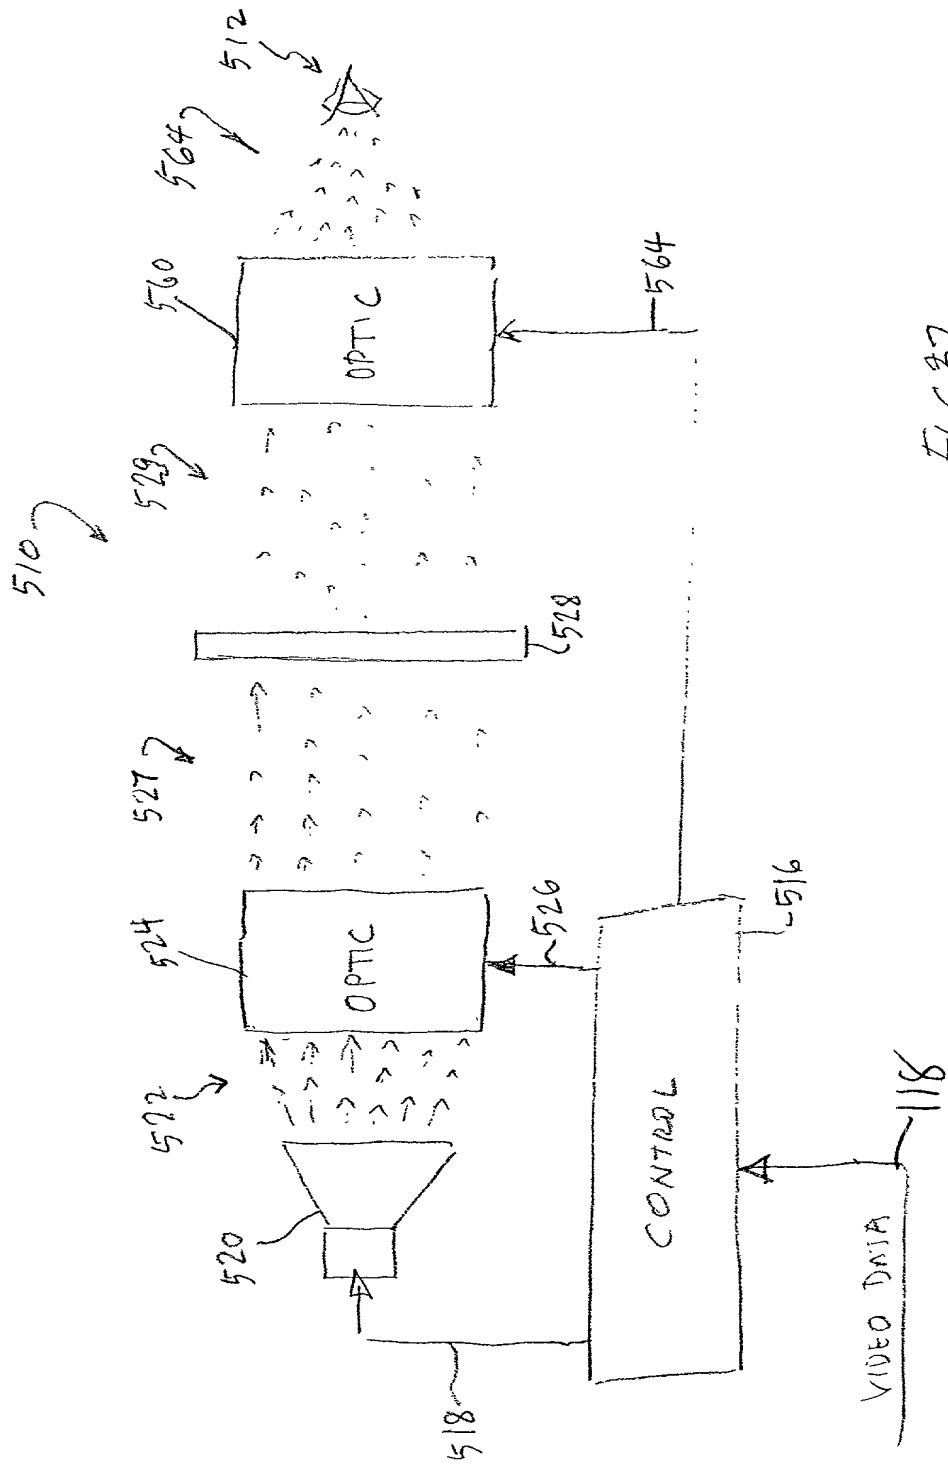


FIG 37

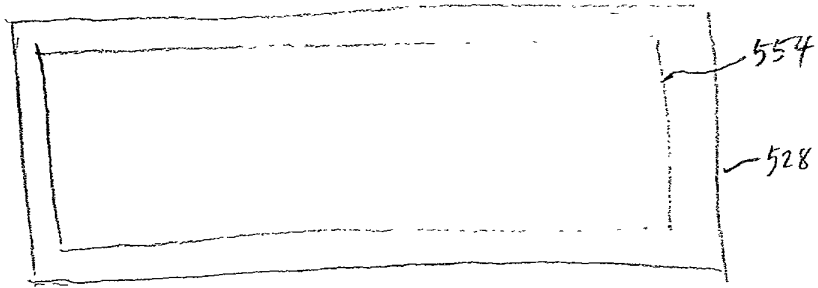


FIG 38

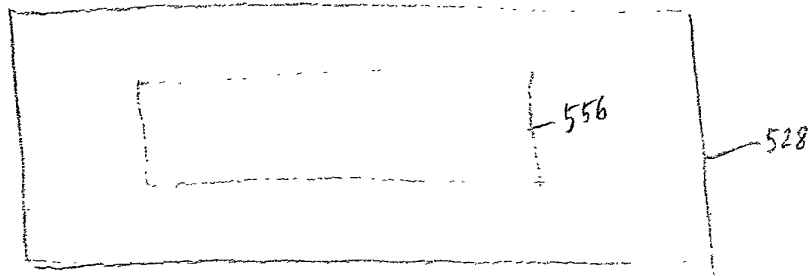


FIG 39

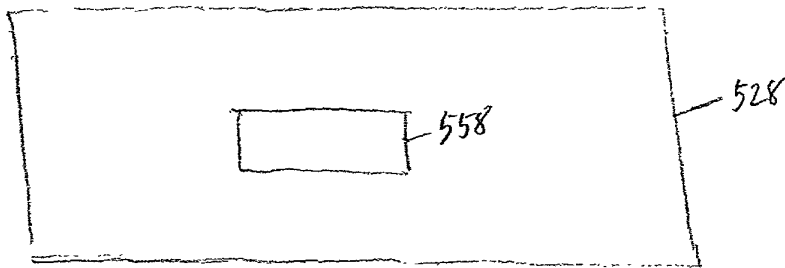


FIG 40